

# Cooperative and Interactive Control Systems in Biomedical Engineering

Günther Schmidt

Thomas Fuhr and Robert Riener

*Interactive Systems and Control Group (ISAC)*




---

Institute of Automatic Control Engineering, Technische Universität München  
Univ.-Professor Dr.-Ing. Dr.-Ing. h.c. Günther Schmidt



# Interaction of Human and Artificial System

## Control and Automation in Medicine

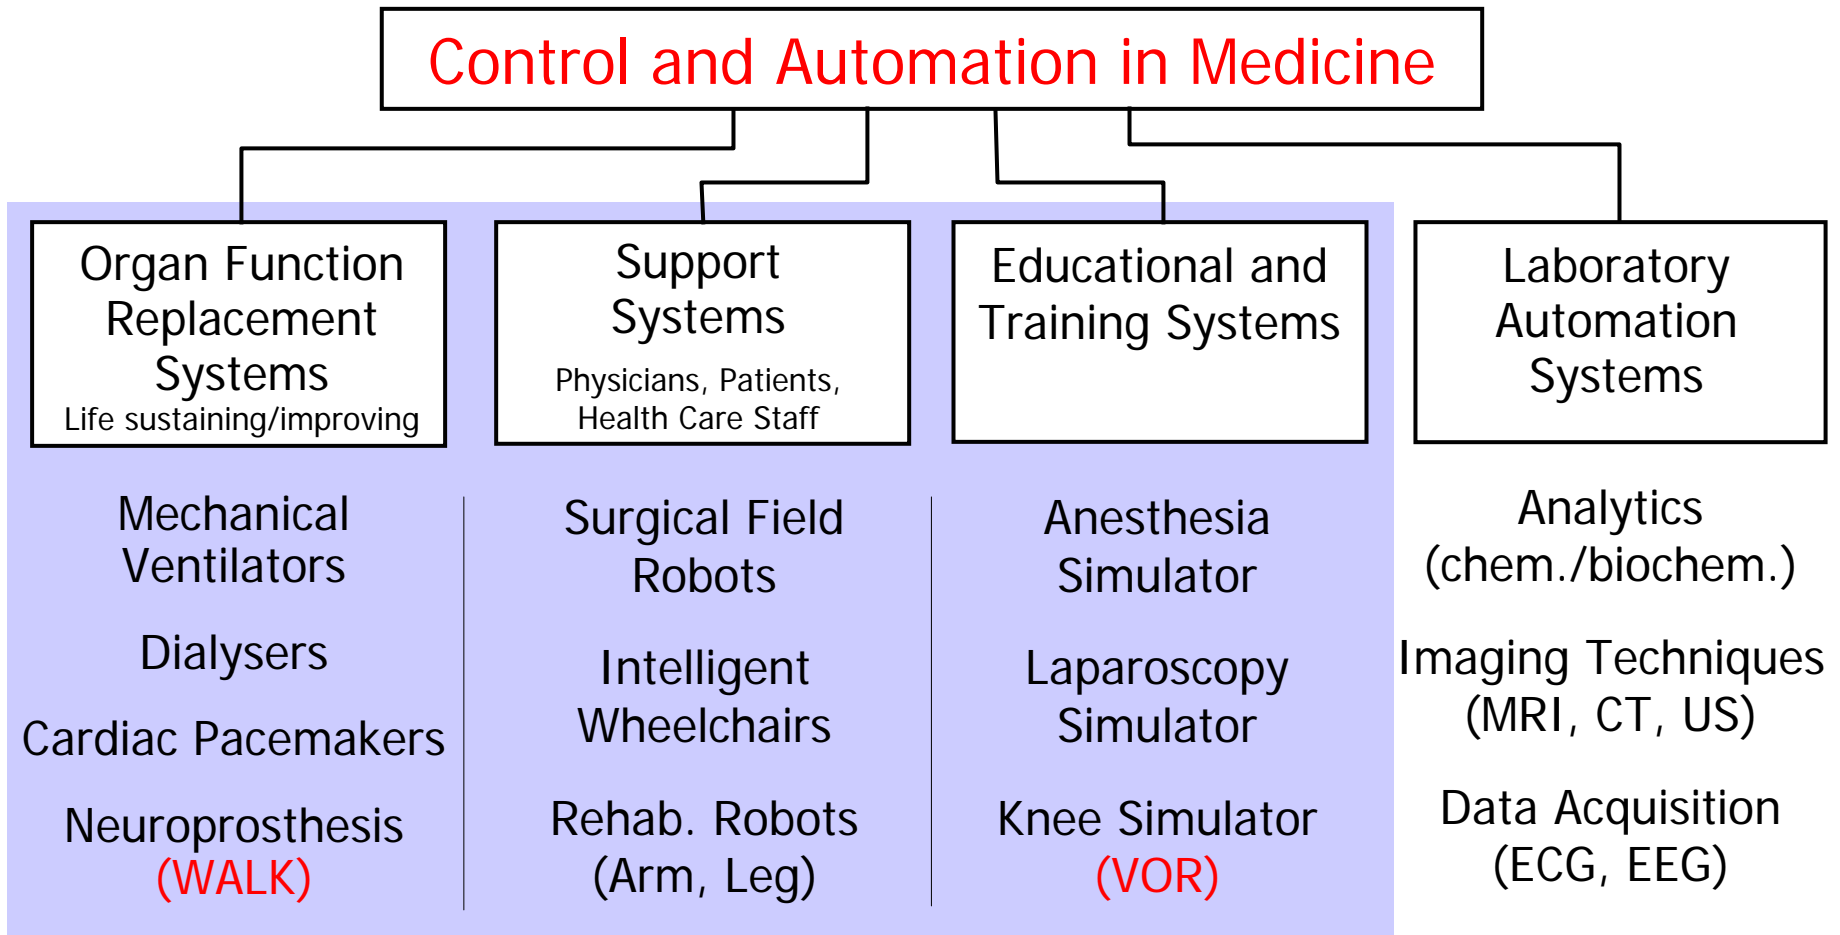

# Definitions

Context: *Human-Centered Controls/Robotics*

- **Cooperativity**

*Human operator is supported by the technical system in executing his/her intentions, but is **not** enforced to do so.*

- **Interactivity**

*Exchange of Information **and** Energy between human and technical system is determined by the human.*

## Research Project #1

# Cooperative Gait Neuroprosthesis





## A Cooperative Gait Neuroprosthesis



Generation of motion patterns  
relevant for locomotion  
by use of  
**Functional Electrical Stimulation  
(FES)**  
of paralyzed limbs



# Gait Neuroprosthesis

## Target Group

- Patients with complete spinal cord injury (thoracic lesions)


## Method

- Electrical stimulation of peripheral motor neurons, surface electrodes

## Relevant Motion Tasks

- **Standing:**  
Standing up, Standing, Sitting down
- **Gait:** Step Forward
- **Stair Climbing:** Stair ascent and descent

## Muscle activation

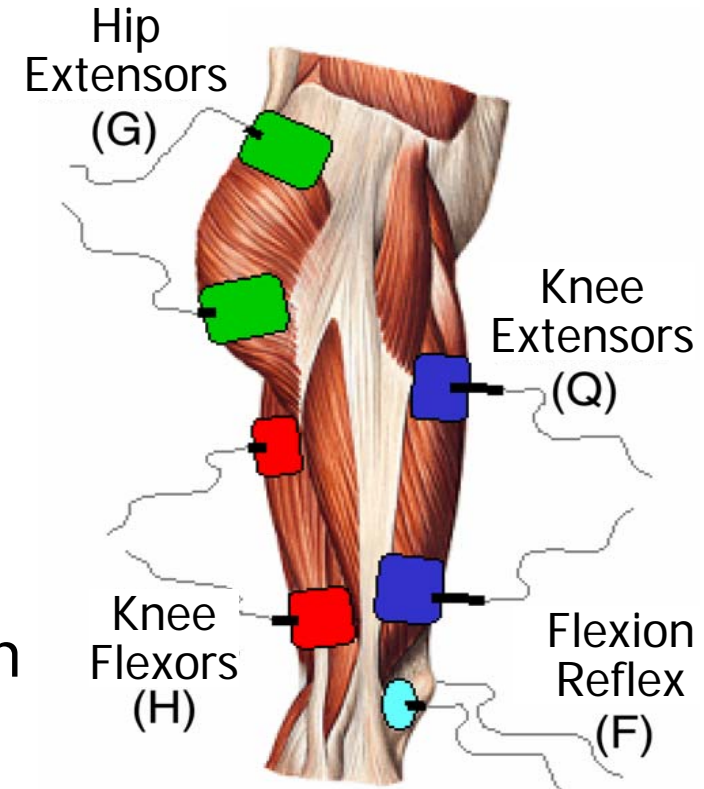



# Gait Neuroprosthesis





## Patient mounted sensors

- Knee angles and angular velocities
- Force sensing soles

# **WALK! System Architecture**

- **Actuators**
  - Technical: neurostimulator, tactile displays
  - Biological: leg muscles, voluntary upper body contributions
- **Sensors**
  - Patient mounted sensor systems: angles, velocities, forces
- **Motion control and supervision, monitoring**
  - Control system, signal processing and data acquisition, user interface

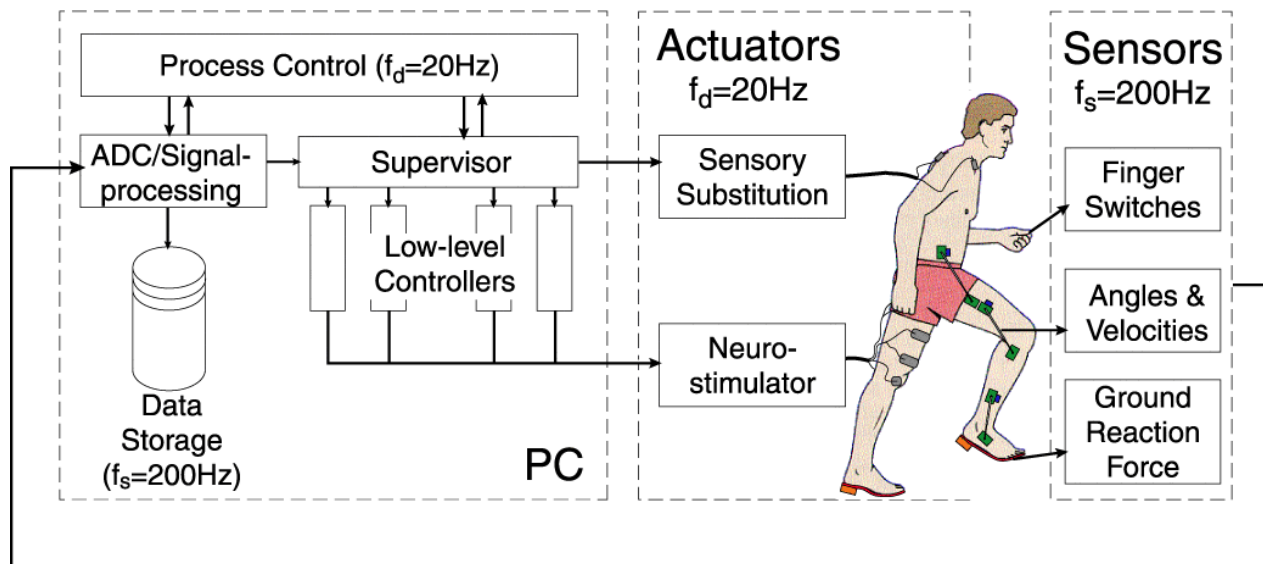



# Control System Challenges

## Plant: *Human Motor System*

- Nonlinear, time-variant: muscle fatigue
- Underactuated: few, coupled stimulation channels
- Unknown plant characteristics
- Competition with voluntary upper body forces
- Control sampling rate: 20 Hz, due to stimulation rate limits

## Requirements:


- **Cooperativity**: neuroprosthesis supports patient
- Maximum safety and reliability
- Minimum complexity




# Hierarchical Control Structure

- Intention level
  - Selection of **motion task** for a specific motion
- Coordination level
  - Discrete event specification of motion tasks by means of a set of **motion phases**
- Activation level
  - Muscle **activation** via low-level open-loop and closed-loop controllers


Intention  
Level

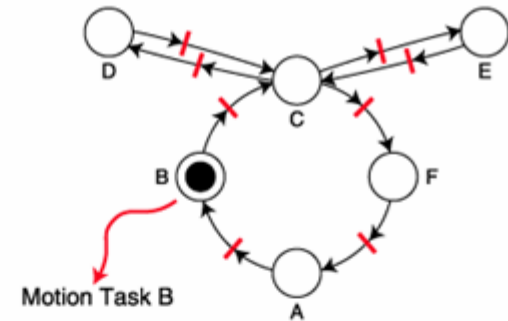

Coordination  
Level

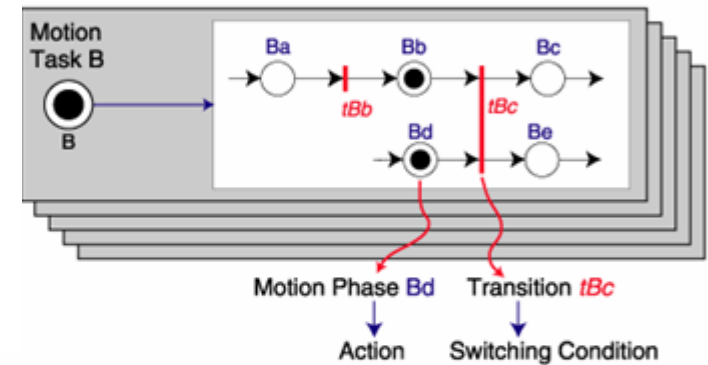


Activation  
Level

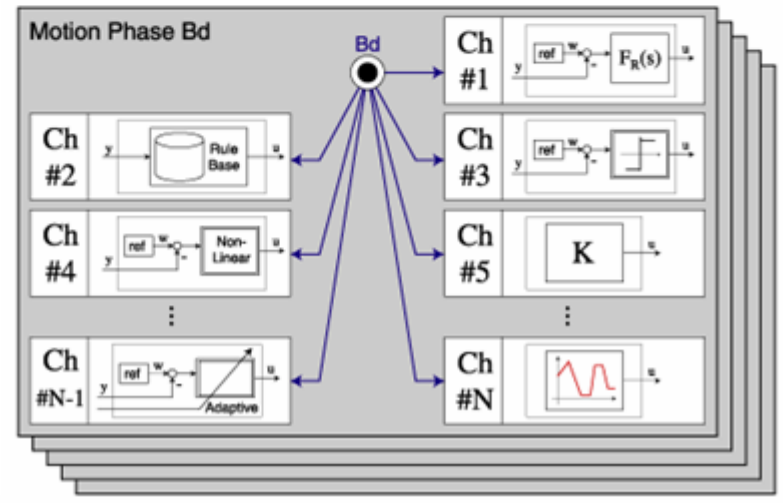


# Motion Task Synthesis



## Step

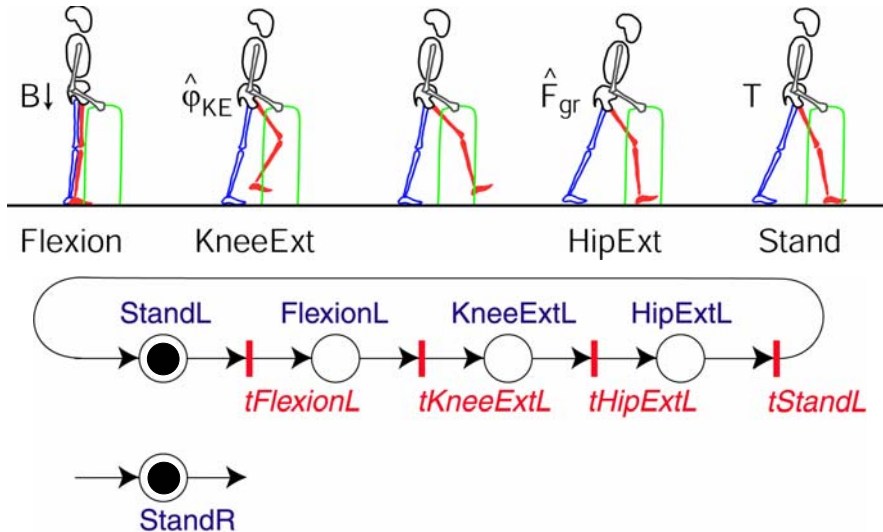

## Stair Ascent

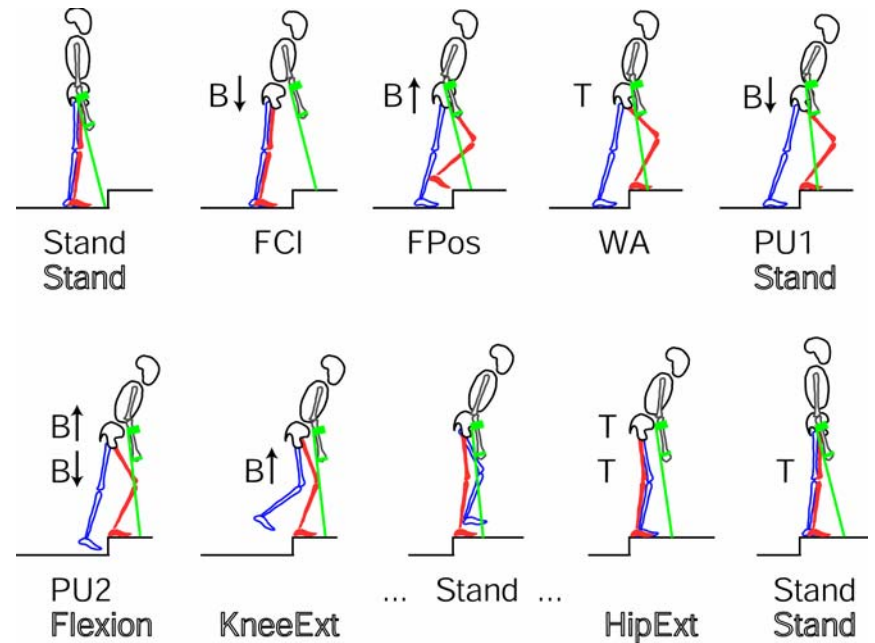


## Knee Extension Controller

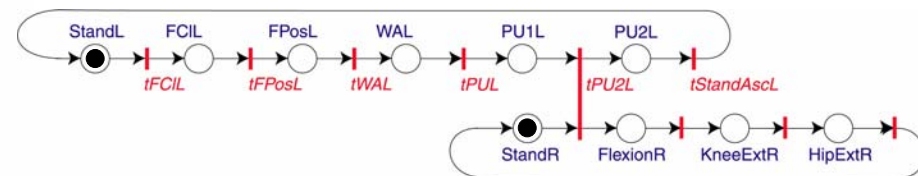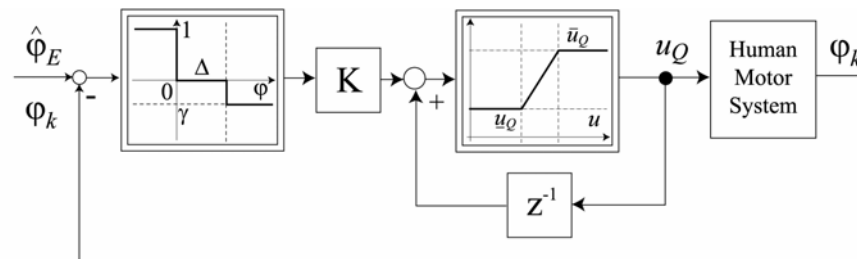

# Knee Extension Control

## Closed-loop control of knee extensor activation (Q):

- (1) Unloaded swing leg is slightly flexed prior to step
- (2) Stand leg supports > 75% of body load
- (3) Knee is slightly flexed during contralateral step

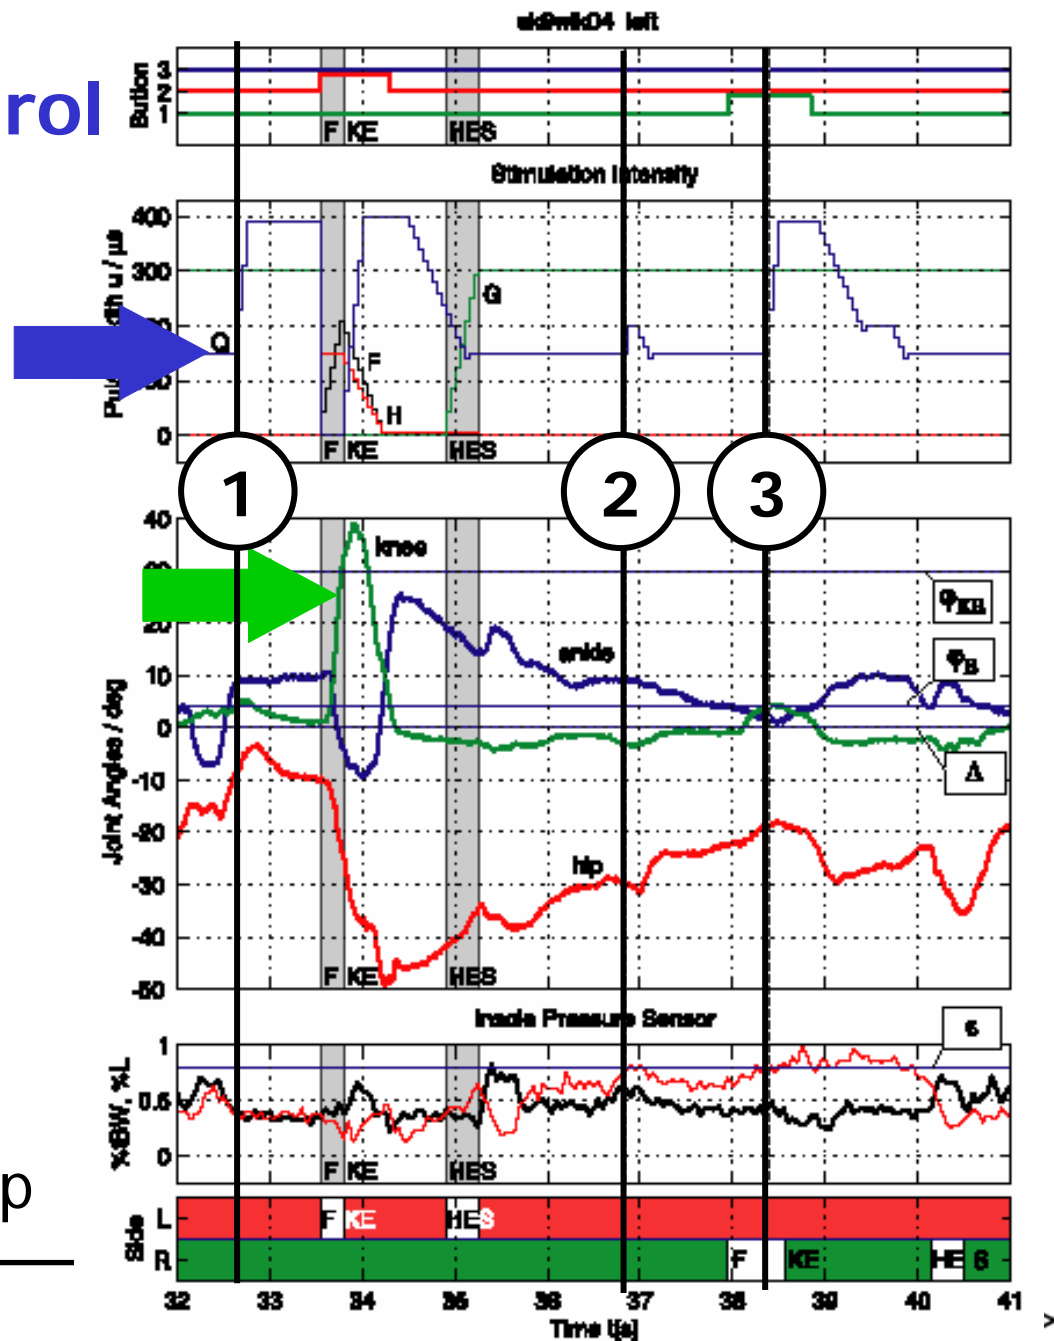




## Supervisor

- CIPN Model
- Resulting from **fusion** of intention level and coordination level

## Elements

- Sensor or switch-triggered **transitions**
- Actions represented by **places**
- Lower-level **controllers**

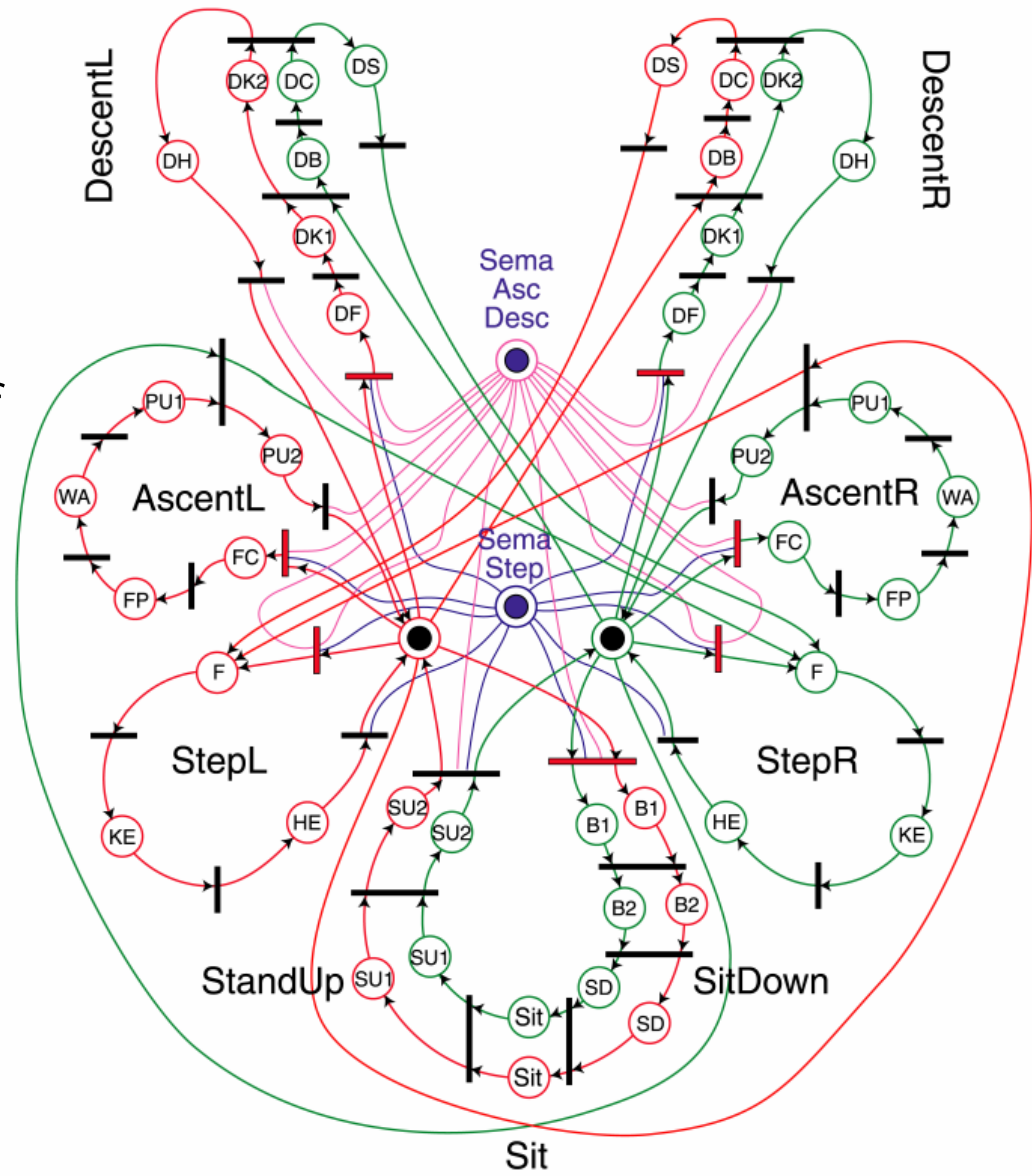




# Cooperative Neuroprosthesis WALK!



- Neurostimulator (ProStim8, FRA)
- Multisensory system
- Sensory substitution system
- Process supervision & control

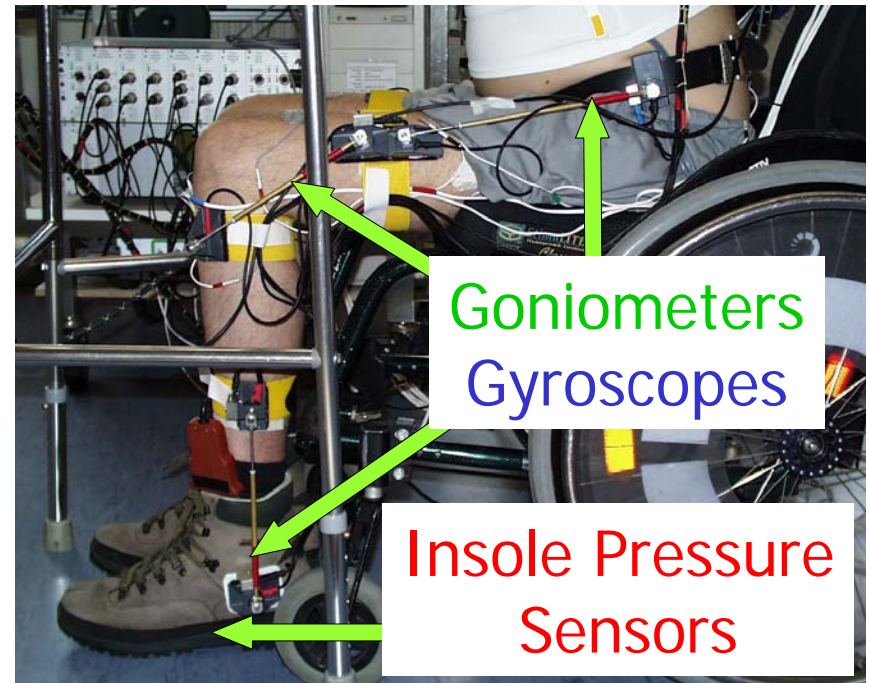

# Welcome to Walk!

A Closed-loop Controlled  
Neuroprosthesis  
to Restore Ambulation



© 2000 Thomas Fuhr

Lehrstuhl f. Steuerungs- und Regelungstechnik  
Technische Universität München

e-mail: [thomas.fuhr@ei.tum.de](mailto:thomas.fuhr@ei.tum.de)







# Stair ascending with closed-loop controlled neuroprosthesis



(a)



(b)



(c)

Step height Platform:  
12.0 & 16.5 cm

Step height Staircase:  
17.0 cm



(d)



(e)



(f)

# Ascending a Staircase with WALK!



# Résumé

- Prerequisite of cooperativity:
  - Merging of methods from area of systems & control, biomechatronics and IT
- Cooperativity of a neuroprosthesis
  - Improves control of movements
  - Releases patients from tasks that can be automatized
  - Reduces muscle fatigue and stimulation intensity
  - Improves patient's quality of life

## Research Project #2


# VR Knee Joint Simulator



# VOR

## Virtual Orthopedic Reality

Multimodal simulator  
for intensive and realistic  
medical education and  
training of clinical  
treatment methods

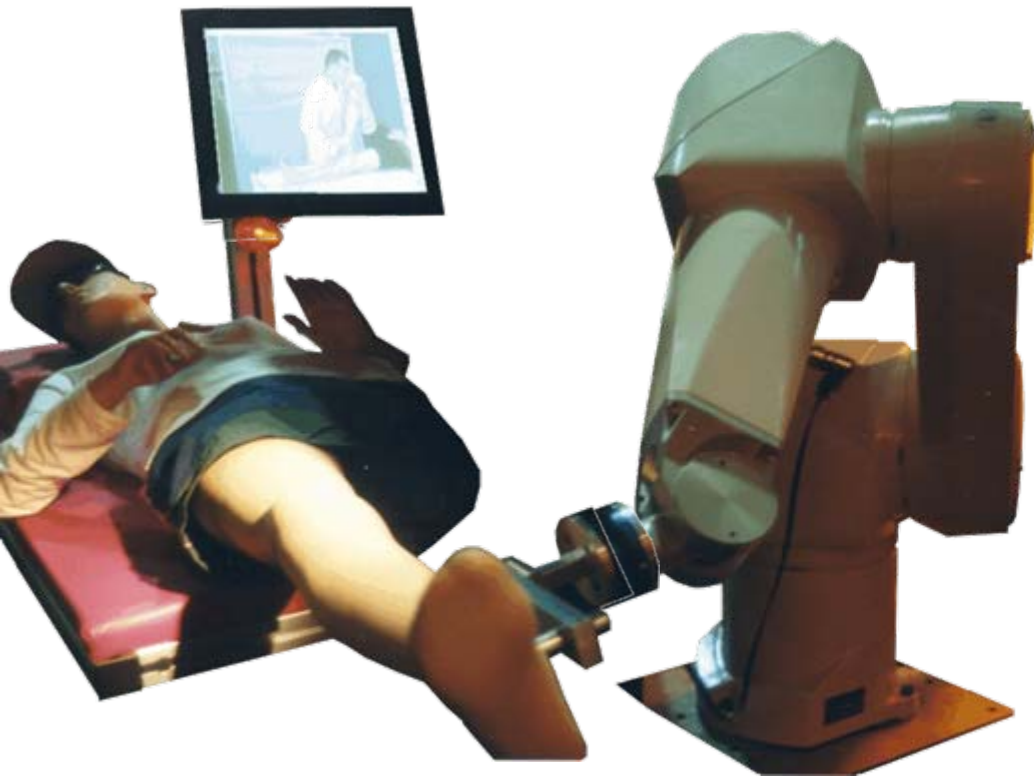

# New Methods in Orthopedic Education

- Joint diagnosis requires high level of experience and sensitivity
- Training with patients is cumbersome, time consuming and expensive
- Result of survey with > 50 orthopedic doctors:  
“ .... training methods need to be improved .... ”




*McMurray Test*  
for diagnosis of  
meniscus injuries



# The Munich Knee Simulator

... a *multimodal* platform for the **interactive** training


- Industrial robot with F/T sensor for *kinesthetic* feedback (highly dynamic)

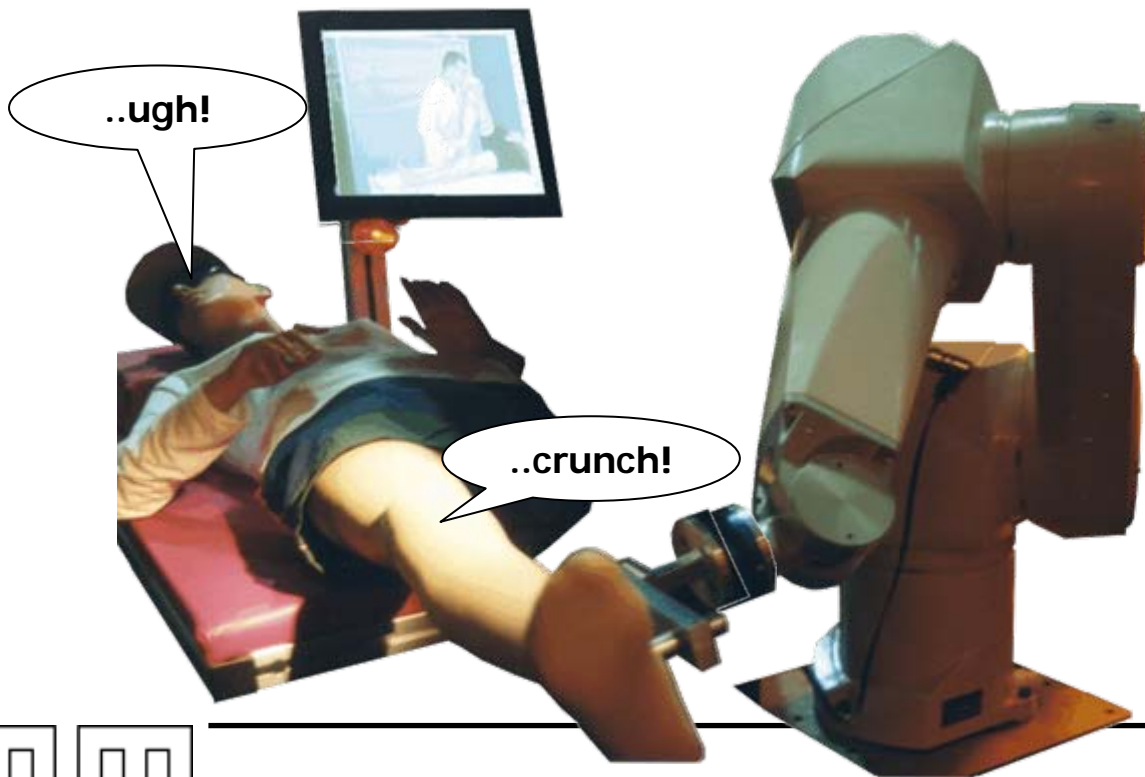

- Artificial leg for *tactile* feedback
- Realistic examination environment
- *Visual* feedback
- *Auditory* feedback




# Principle of Multimodal VR

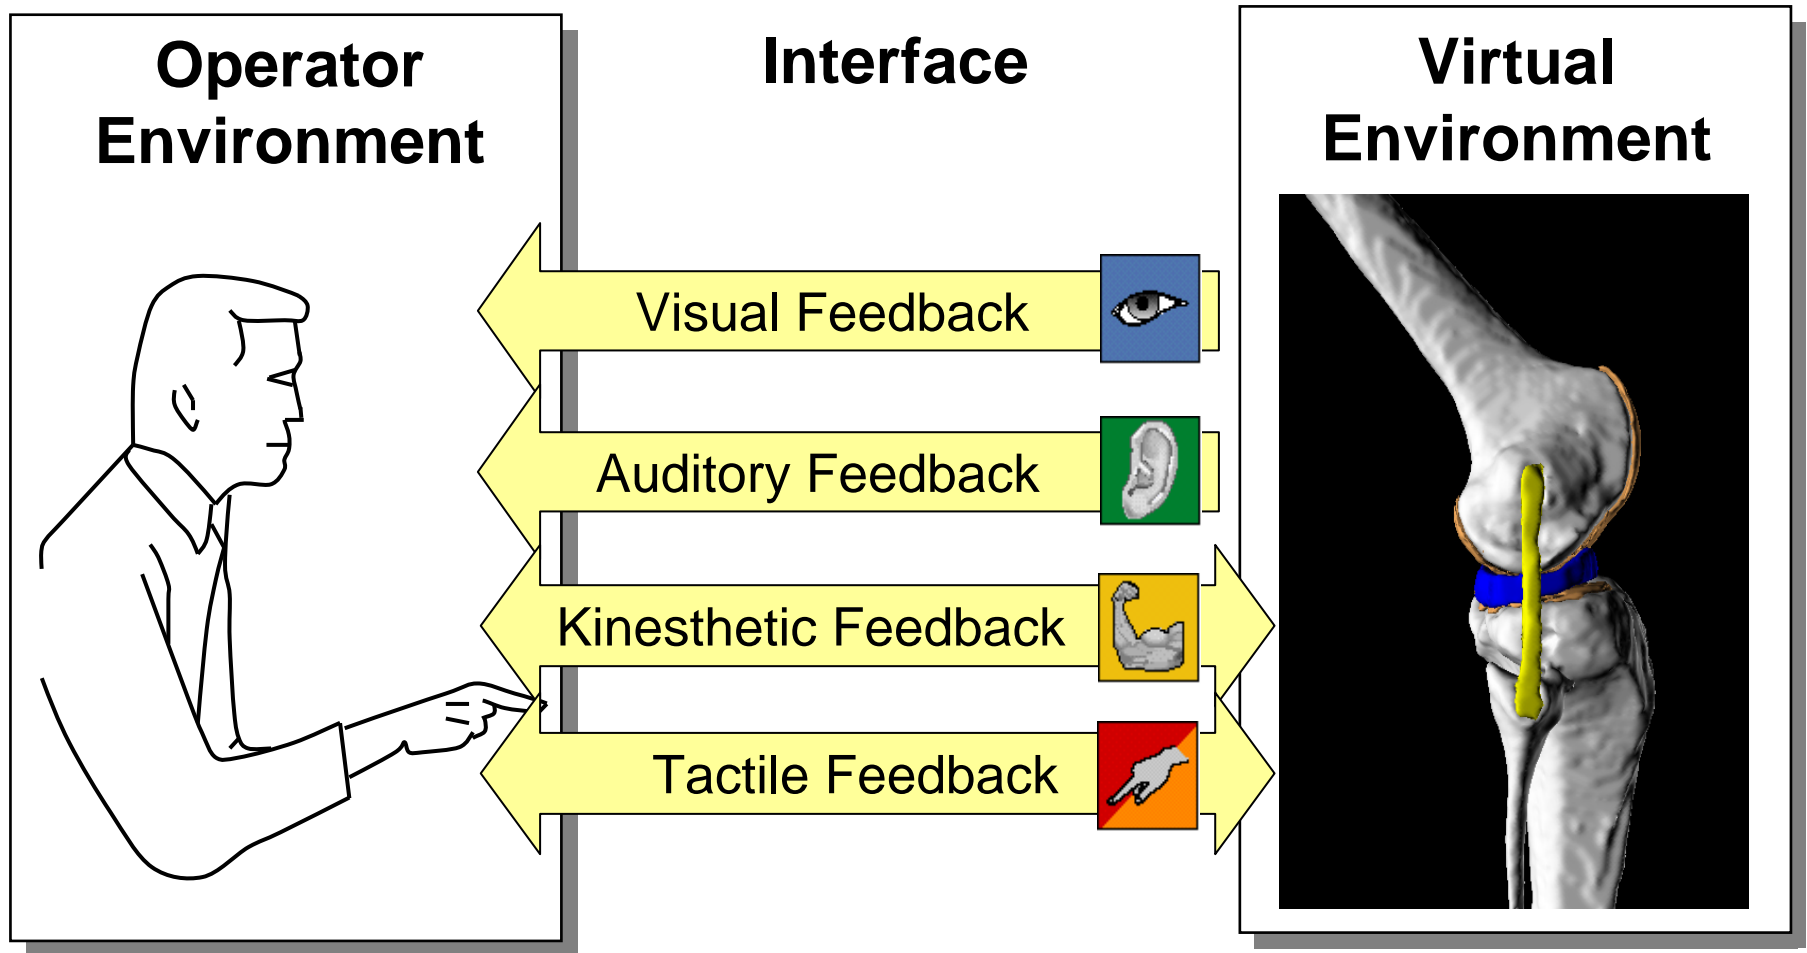

# Operational Modes

## #1 Teaching Mode: Artificial leg performs desired motion

- Operator learns appropriate test movements in 6 DoFs through motion playback

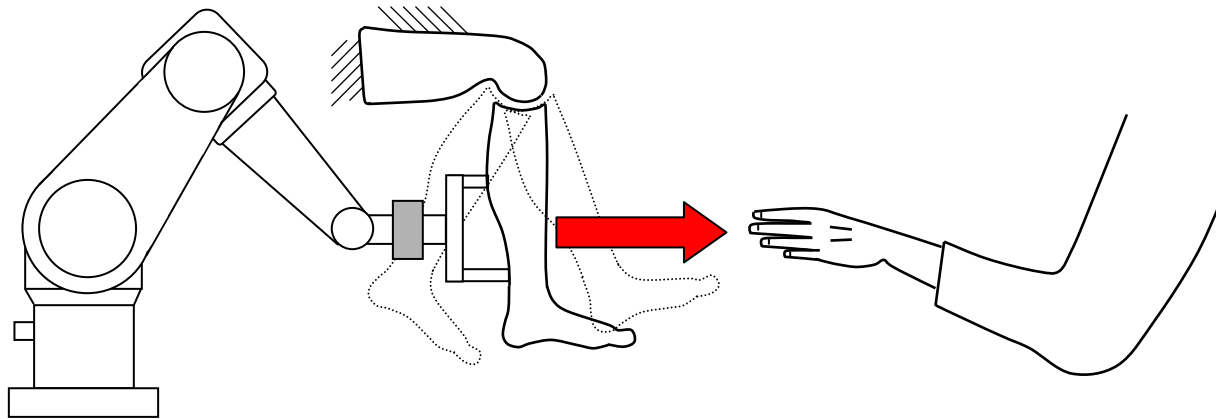




# Data Acquisition for Teaching Mode

Analysis of 60 functional tests, executed by an experienced orthopaedian

## Motion tracking system

- 3 video cameras
- 4 electromagnetic position sensors

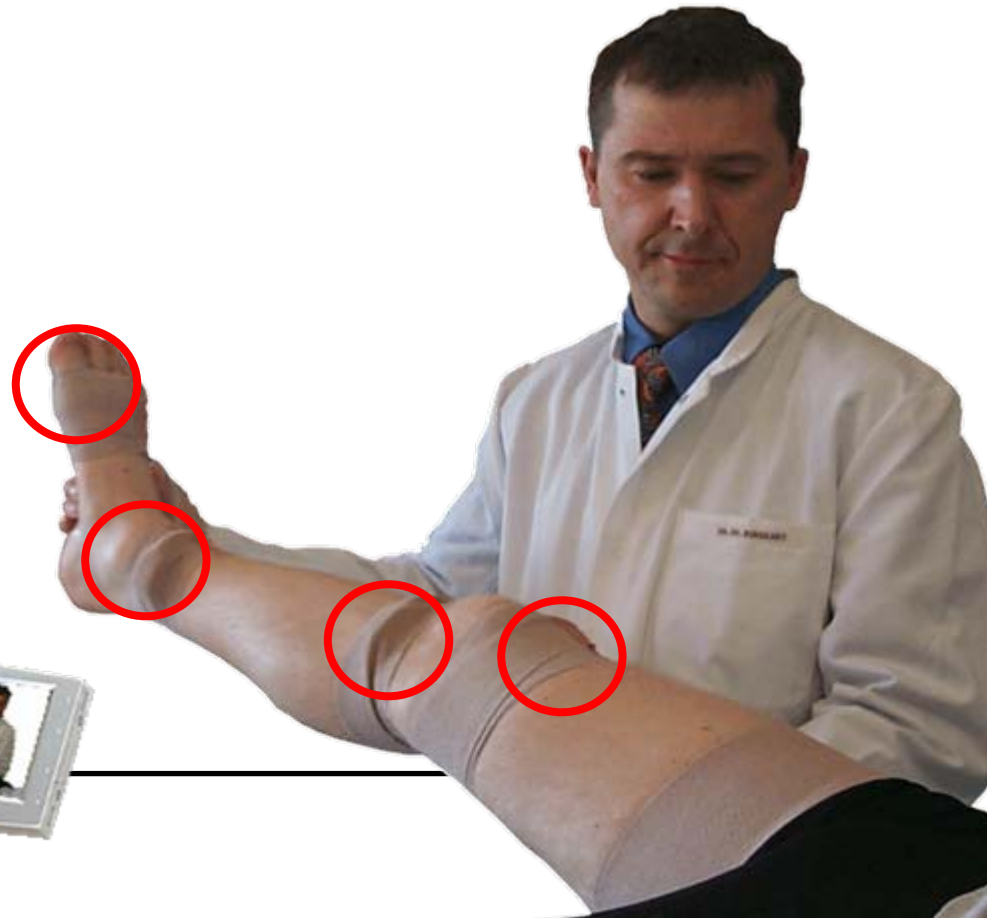


# Operational Modes

#1 Teaching Mode: Artificial leg performs desired motion

- Operator learns appropriate test movements in 6 DoFs

**#2 Interactive Mode: Artificial leg reacts to operator interaction**

- Operator perceives (simulated) physiological/pathological properties of knee joint mechanics in 6 DoFs

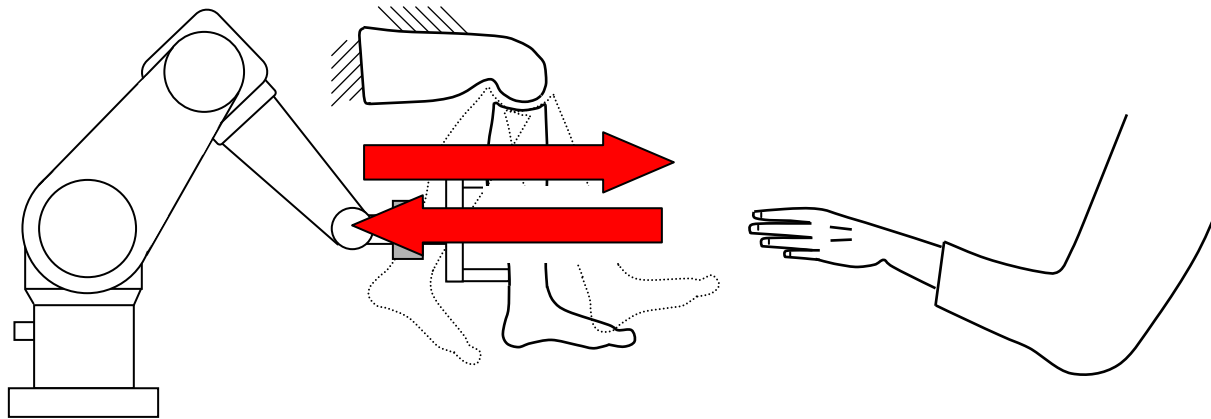


# Interactive Mode A



# Interactive Mode B


**Admittance control enables force reflection in 6 DoFs**

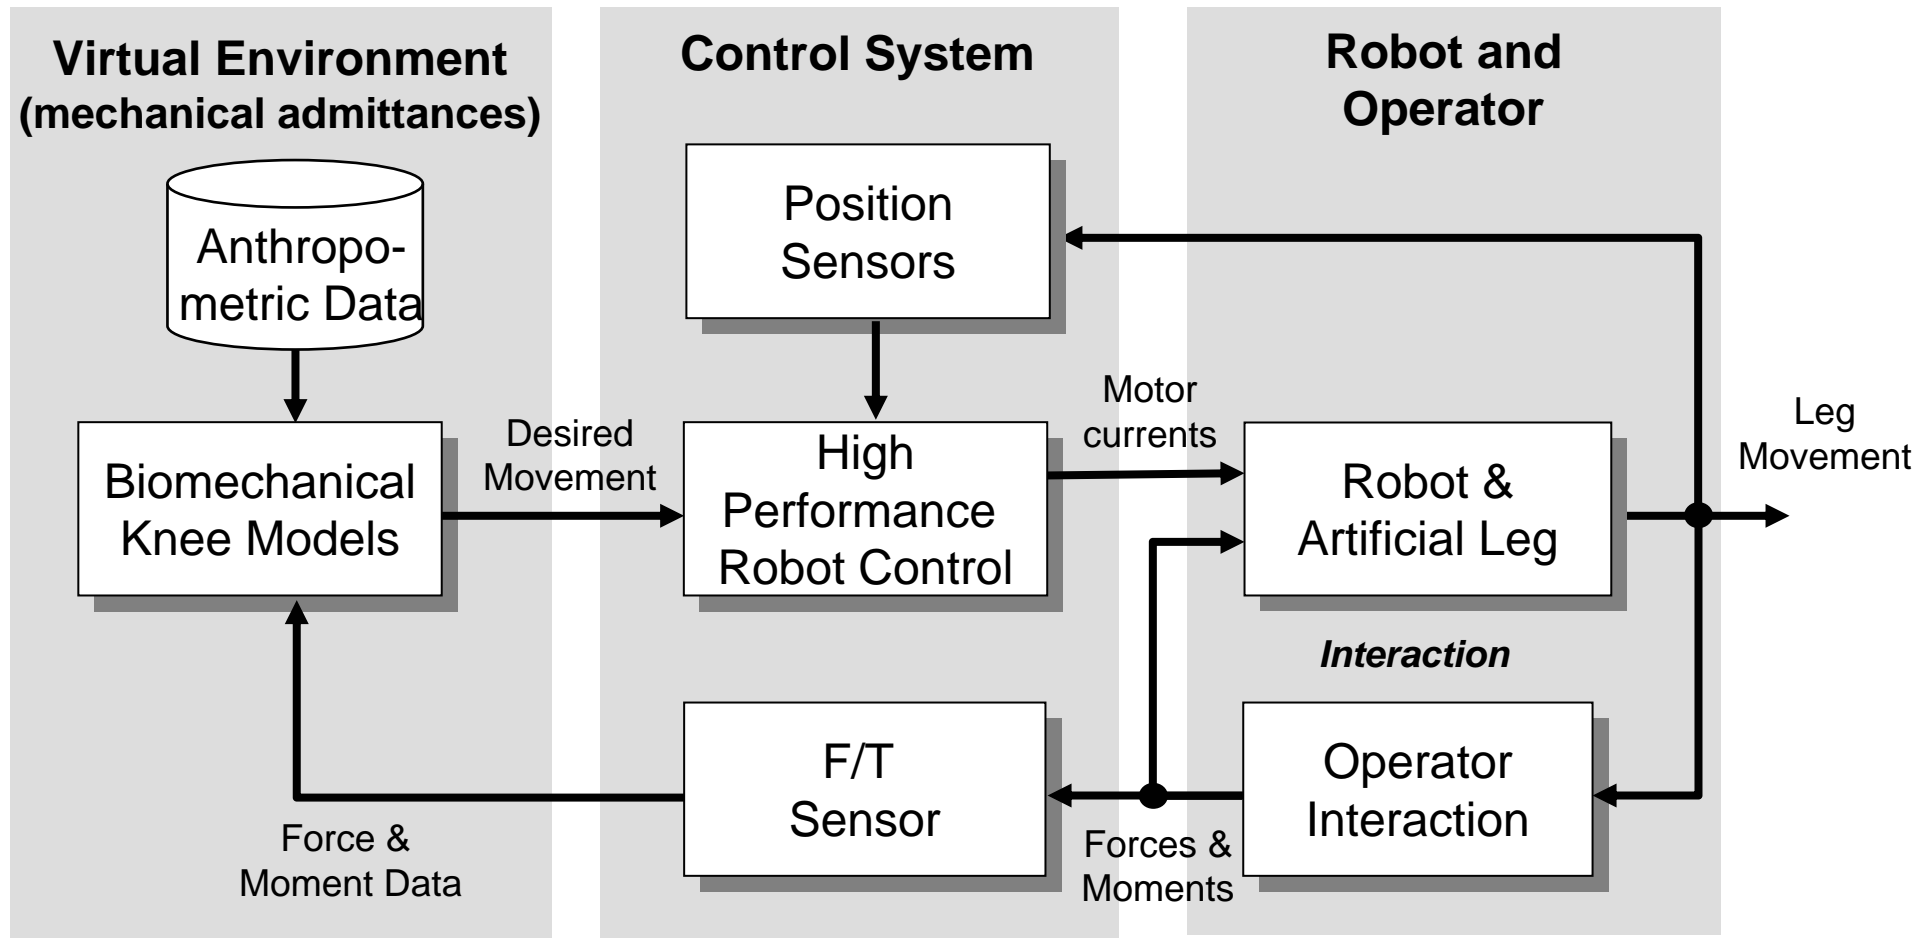

# Network Model of Kinesthetics

● Impedance  $f(t) = Z(x(t))$       ● Admittance  $x(t) = Y(f(t))$

● e.g. linear:  $x(s) = \frac{1}{ms^2 + ds + k} \cdot f(s)$

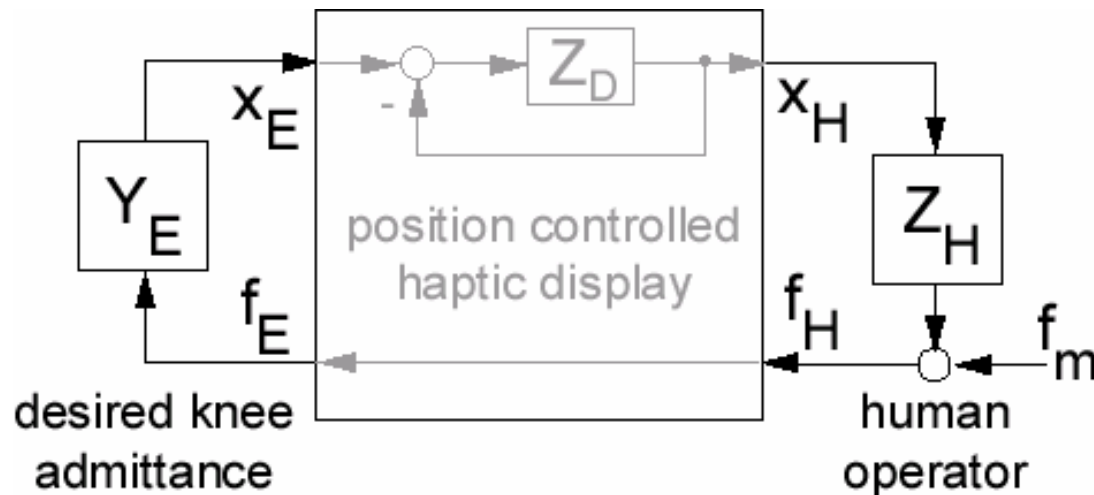

● Control Objectives : Stability & Transparency

i.e.  $f_H = f_E$  &  $x_H = x_E$



# Admittance Control System and Robot Kinetics

Robot Model  $M(q)\ddot{q} + F(\dot{q}) + G(q) = \tau_A - J^T f_H$

+

Control Law  $\tau_A = r + k$

Model-based  
Compensator  $k = \hat{F}(\dot{q}) + \hat{G}_g(q) + \hat{G}_s(q_2) + J^T f_S$   
 $\hat{F}_i(\dot{q}_i) = c_v \dot{q}_i + c_c \text{sign}(\dot{q}_i) , f_S = f_H$

SFB/FF  
Controller  $r = \hat{M}(\ddot{q}_d + K_v(\dot{q}_d - \dot{q}) + K_p(q_d - q))$

Kinematics  $\begin{bmatrix} \dot{x}^q & \dot{y}^q & \dot{\theta}^q \end{bmatrix} = \text{JWSKJWS} \begin{bmatrix} \dot{x}^q & \dot{y}^q & \dot{\theta}^q \end{bmatrix}$



Biomechanics  $x_d = x_E = Y(f_E)$



# Prototype of the Knee Simulator



# Acquisition of Biomechanical Knee Data

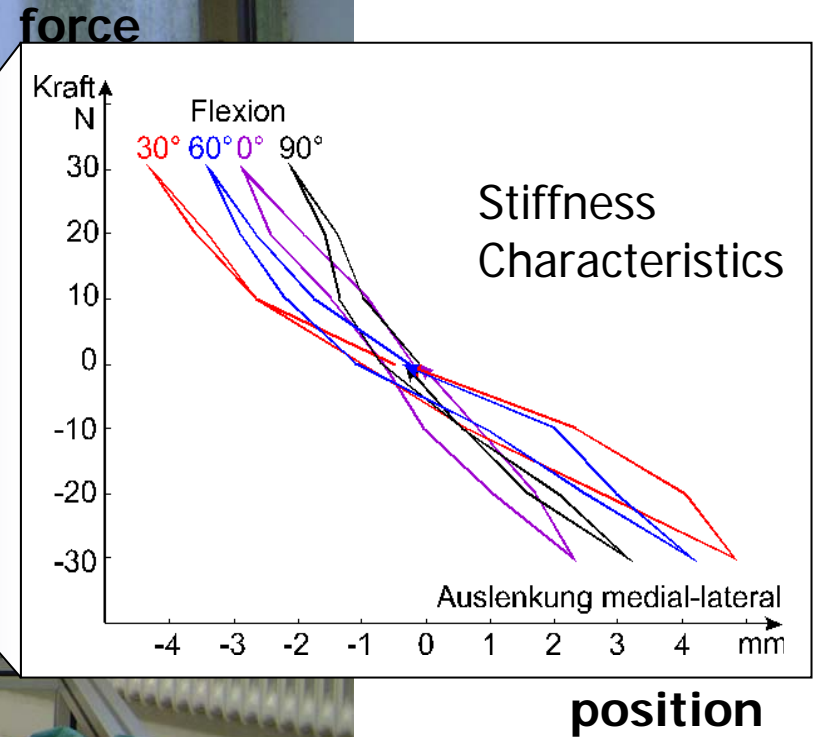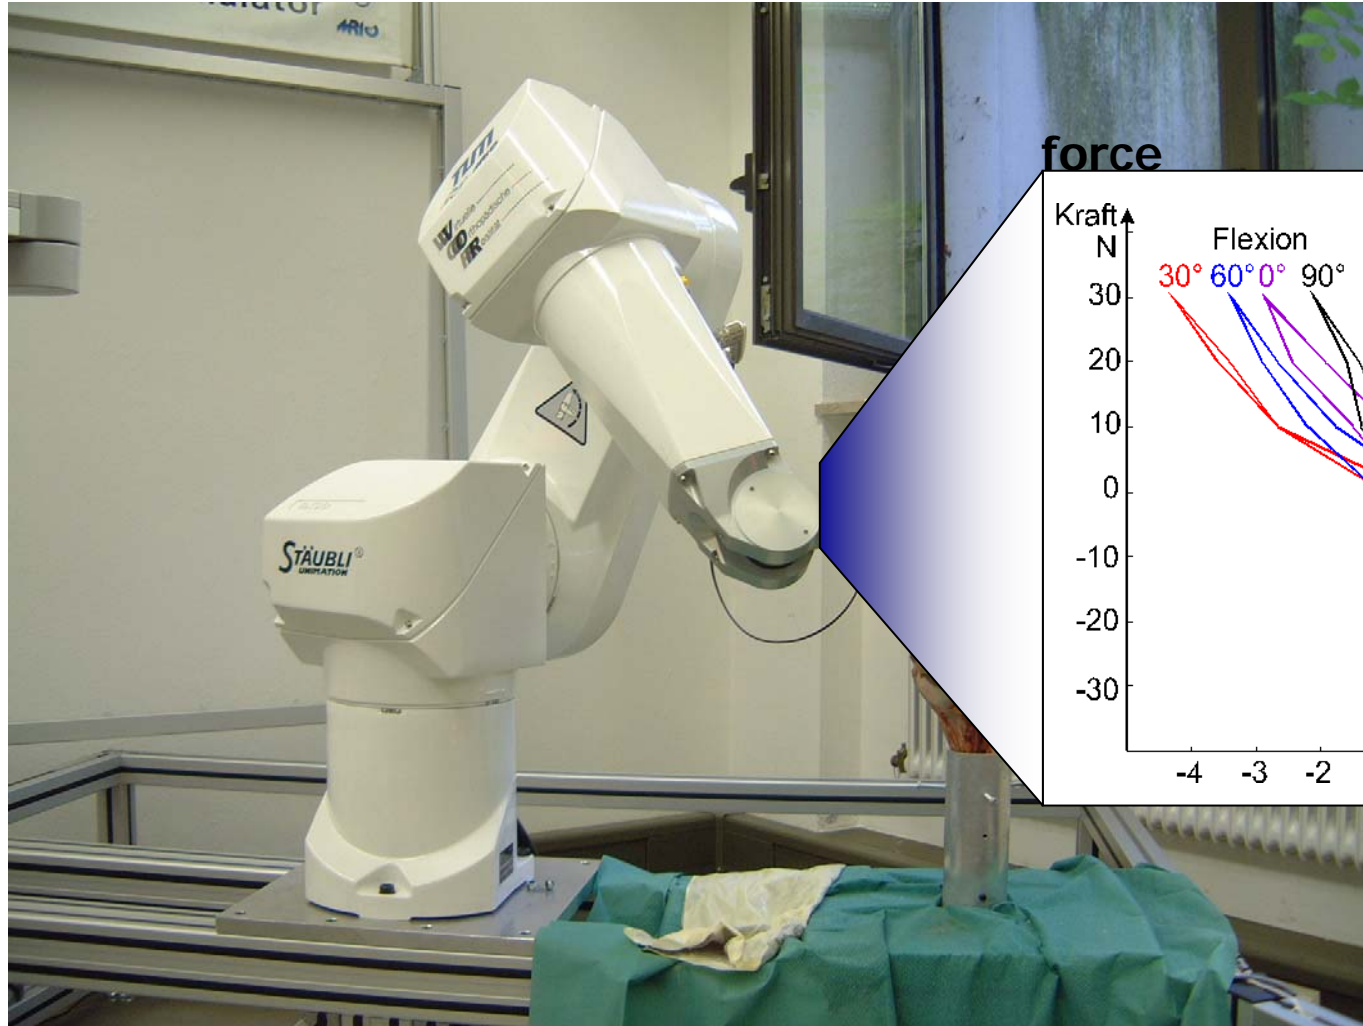

# Résumé

- Prerequisite of **interactivity**:
  - Blending of methods from area of **systems & control, biomechatronics** and **IT, VR**
- Interactivity of the **knee simulator** supports
  - realistic, multimodal simulation of knee pathologies
  - more intensive and practical medical training

## Outlook


**Transfer** of technological know-how into related application fields, e.g. ....

# Delivery Training Simulator


for medical students and midwives

## Cooperation partners at TUM

- LSR: R. Riener, F. Frey
- Orthopedic Clinic:  
R. Burgkart, T. Obst
- Clinic for Gynaecology:  
E. Ruckhäberle, K.  
Schneider

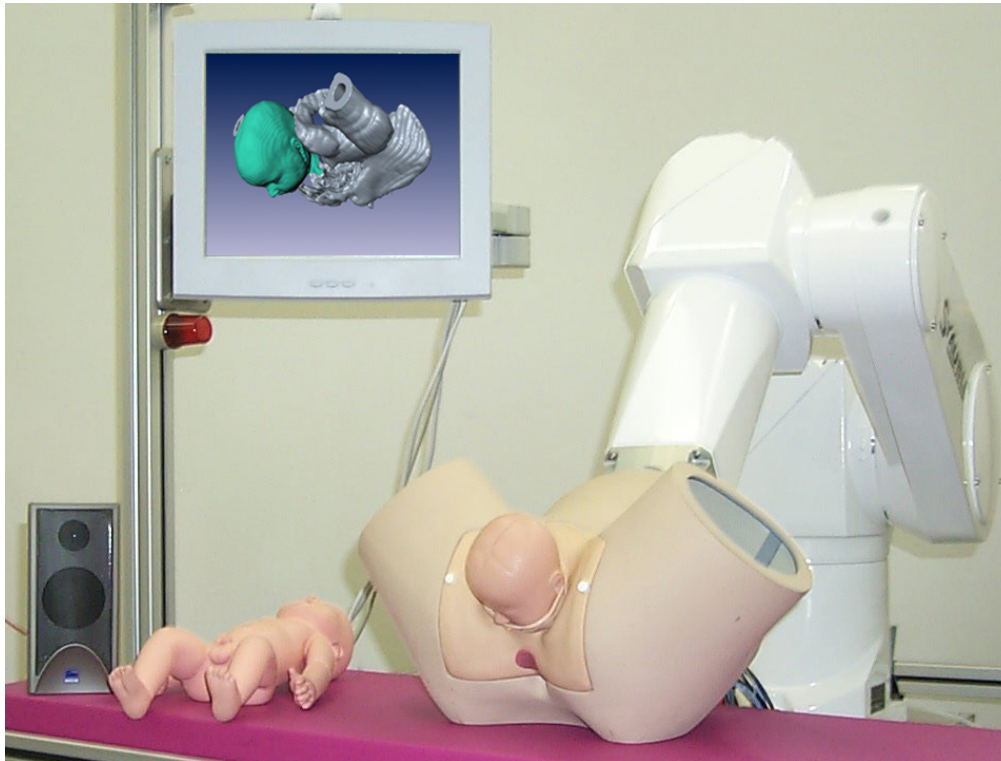

Baby passing through cervix without  
and **with** doctor's intervention

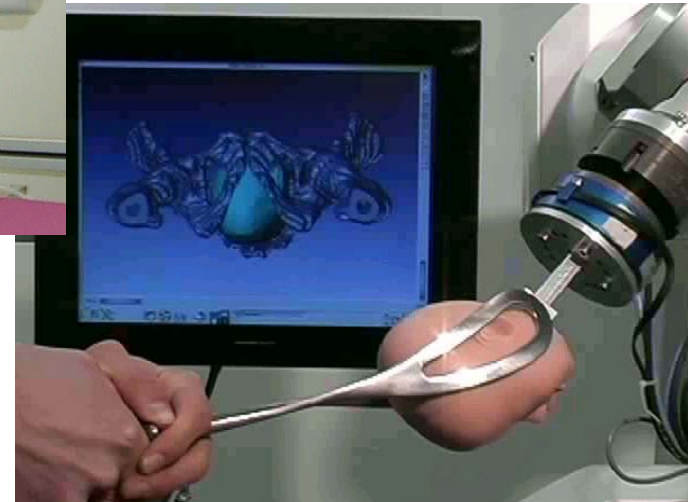

# Conclusions from Projects

- Prerequisite for achieving cooperativity or interactivity:
  - Blending of methods from areas of automation, systems & control, biomechatronics, VR and IT
- Cooperativity of a neuroprosthesis
  - Improves control of movements
  - Releases patients from tasks that can be automated
  - Reduces muscle fatigue and stimulation intensity, ...
- Interactivity of the knee simulator supports
  - Realistic, multimodal simulation of knee pathologies
  - More intensive and practical medical training

*Thank you  
for your attention*

